





2 Fluke Corporation 1523 € , f ,  
øùPB


- 1523 0.3
- 1524 0.3

1523

- 1523 1524
- 1524

1523 1524

128x64

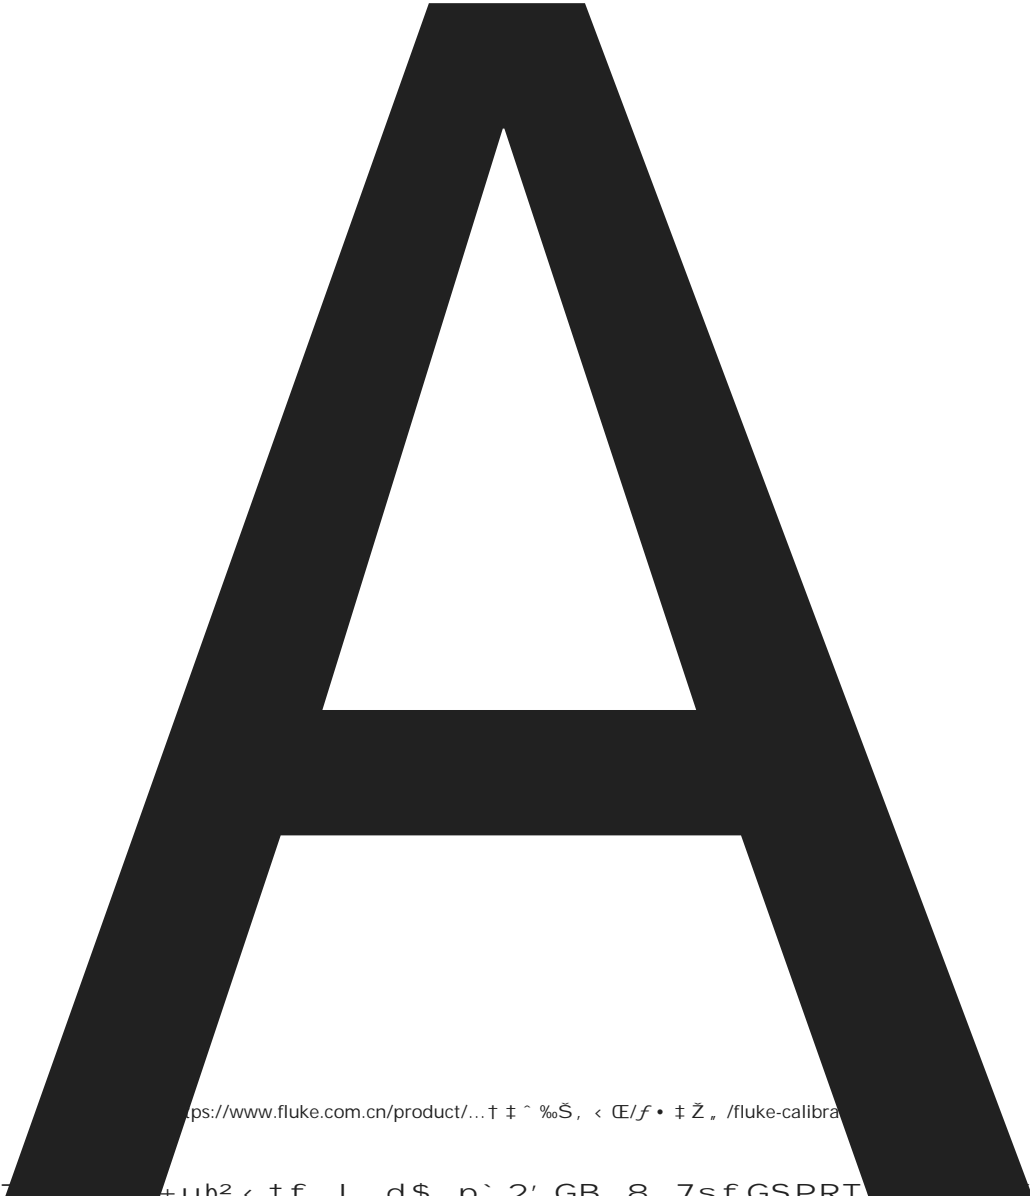





420 C

5616-12: 0.050  
5615-6S d â  
5627A-12: 0.130  
5610-9S d â

F á PÔœ÷ • ÓI @ ‡ ^ - I @ !

PRTÌ Í ' ' ½' Î Ì ĐÑÒ» Ó

-100 C	0.011
0 C	0.015
100 C	0.019
200 C	0.023
400 C	0.031
600 C	0.039

É Ù Ê Û Ì Í ' ' ½' Î Ì ĐÑÒ» Ó

0 C	0.002
25 C	0.003
50 C	0.006
75 C	0.014
100 C	0.030

# Ordering information



Fluke 1523

Fluke 1523 200 t 660 C 25" # \$ INFO-CON ? @ÓTPAK - 4ùF

~~Fluke 1523-P2~~

1523 5628 PRT • 200 C 660 C 25" # [1/4 x 12 \$ ] Ó" â i ¥ c INFO-CON ? @ÓTPAK - 4ùF

**Includes:**

U , p...P % 7` bU` 7` b f "gá ô < 4ùF

Includes:

- Universal TC INFO-CON Connector
  - TPAK
  - Case
-